

R9400

REED INSTRUMENTS

Carbon Monoxide Meter with Temperature



Instruction
Manual



Table of Contents

Introduction	2
Product Quality	3
Safety	3
Features	4
Specifications	4-5
Included	5
Instrument Description	6
Display Description	6
Operating Instructions	7-8
<i>Unit of Measure Selection (Temperature)</i>	7
<i>Data Hold</i>	7
<i>Setting the Alarm Threshold</i>	7
<i>MAX Function</i>	8
<i>Auto Power Off</i>	8
<i>Backlight</i>	8
<i>Beeper Off</i>	8
Battery Replacement	9
Accessories and Replacement Parts	9
Applications	9
Product Care	10
Product Warranty	10
Product Disposal and Recycling	10
Product Support	11

Introduction

Thank you for purchasing your R9400 Carbon Monoxide Meter with Temperature. Please read the following instructions carefully before using your instrument. By following the steps outlined in this manual your meter will provide years of reliable service.

Product Quality

This product has been manufactured in an ISO9001 facility and has been calibrated during the manufacturing process to meet stated product specifications. If a certificate of calibration is required please contact the nearest authorized REED distributor or authorized Service Center. Please note an additional fee for this service will apply.

Safety

Never attempt to repair or modify your instrument. Dismantling your product, other than for the purpose of replacing batteries, may cause damage that will not be covered under the manufacturer's warranty. Servicing should only be provided by an authorized service center.



Carbon monoxide (CO) can be life threatening even at relatively low concentrations. Do not use this meter as a personal safety monitoring device.

**For safety reasons, we recommend
that this unit be certified every year.**

Effects of Carbon Monoxide (CO) Poisoning

0 to 1ppm	Normal background levels
9ppm	ASHRAE Standard 62-1989 for living areas
35ppm	The average exposure level per U.S. OSHA workplace standards
50ppm	OSHA enclosed space 8-hour average level*
100ppm	OSHA exposure limit*
200ppm	Mild headache, fatigue, nausea and dizziness
400ppm	Headache occurs in 2.5 to 3.5 hours
800ppm	Dizziness, nausea and convulsions, Death within 2 to 3 hours

* U.S. Department of Labor, Occupational Safety & Health Administration (OSHA) Regulation 1917.24: The CO content in any enclosed space shall be maintained at not more than 50ppm (0.005%). Remove employees from enclosed space if the CO concentration exceeds 100ppm (0.01%).

Features

- Backlit LCD displays CO levels from 0 to 1000ppm and ambient temperature
- User adjustable alarm limit (audible beep frequency increases as CO level rises)
- Quick response and high accuracy
- Data hold and max functions
- Self test sequence on start-up
- Low battery indicator and auto shut off

Specifications

Carbon Monoxide

Measuring Range:	1 to 1000ppm
Accuracy:	±5% or ±5ppm
Resolution:	1ppm
Sensor Type:	Stabilized electrochemical sensor

Temperature

Measuring Range:	-4 to 158°F (-20 to 70°C)
Accuracy:	±1.5°F (0.8°C)
Resolution:	0.1°F (0.1°C)
Sensor Type:	Thermistor

General Specifications

Display:	4-digit, dual LCD
Backlit Display:	Yes
F/C Switchable:	Yes
Alarm:	Audible (buzzer)
Alarm Limit:	User Adjustable
Max Hold:	Yes
Display Hold:	Yes
Warm-up Time:	60 seconds

continued...

REED

Response Time:	2x per second
Auto Shut-off:	Yes (after 30 mins, off)
Power Supply:	4 AA batteries
Battery Life:	Approx. 200 hours
Low Battery Indicator:	Yes
Product Certifications:	CE
Operating Temperature:	32 to 122°F (0 to 50°C)
Storage Temperature:	14 to 140°F (-10 to 60°C)
Operating Humidity Range:	10 to 90%
Dimensions:	7.5 x 2.6 x 1.7" (190 x 65 x 45mm)
Weight:	8.3oz (235g)

Included

- Soft Carrying Case
- Batteries


Instrument Description

1. Sensor
2. LCD Screen
3. Data Hold Button
4. MAX/Down Button
5. Power Button
6. Battery Cover
7. Set Alarm Button
8. Backlight Button
9. Unit of Measure/Up Button



Display Description

1. Auto Power Off Indicator
- MAX Indicator
- Data Hold Indicator
- Beeper Off Indicator
- Unit Indicator
- High Alarm Indicator
- Unit Indicator
- Temperature Reading
- SET Alarm
- Alarm Indicator
- CO Reading
- Battery Capacity Indicator

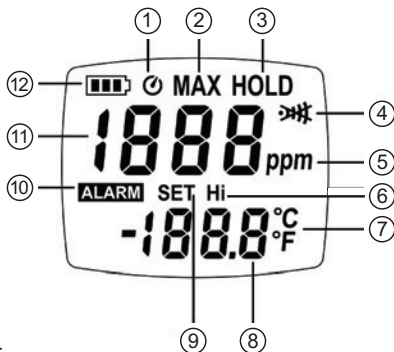

Operating Instructions

1. Push the Power button to turn the meter on. To turn the meter off, press and hold the Power button until the meter counts down from 3 to 0.
2. When turning the meter on it will perform a self-diagnostic test. During the test the LCD will count down from 60 to 0. Once the meter passes the self-test a beep will sound and the meter will begin taking measurements. If the meter does not pass the self-test the LCD will display "Err" and the meter will not take a measurement.

Note: If the meter reads above 1000ppm the LCD will display "OL" to indicate the measurement is out of range.

Unit of Measure Selection (Temperature)

When the meter is powered on press the °C/°F button to toggle between Celsius and Fahrenheit.

Note: The default unit of measure is Celsius (°C). The meter will automatically save the last selected unit of measure when turned off.

Data Hold

Press the **HOLD** button to freeze the current reading on the display. Press the button again to resume normal operation.

Note: When the Data Hold function is enabled the Max and °C/°F buttons are disabled.

Setting the Alarm Threshold

1. Press and hold the **SET** button to set the CO High Alarm Threshold.
2. While holding the **SET** Button, press the Up and Down buttons to adjust the value.
3. Release the **SET** button to save and resume normal operation.

Note: The high alarm is set to 35ppm by default and can be adjusted between 0 and 1000ppm. As the concentration of carbon monoxide rises, the frequency of the beep increases.

continued...

MAX Function

1. When pressing the **MAX** button once, the MAX Indicator will appear on the display. The maximum values (temperature and carbon monoxide) are displayed and will automatically update when new maximum data values are measured.
2. Press the **MAX** button again and the MAX indicator will blink continuously. The Maximum values will automatically update in the Max memory while the current temperature and humidity measurements are displayed. To view the Max measurements during this mode press the **MAX** button at any time to access stored values.
3. To exit MAX mode and resume normal operation, press and hold the **MAX** button for two seconds.

Auto Power Off

To preserve battery life, the meter is programmed to turn itself off after 30 minutes of inactivity. To disable this feature, press and hold the **HOLD** button while powering on the meter. When the meter turns on, release both buttons simultaneously. The Auto Power Off indicator will not appear on the display, confirming this feature is now disabled. If the meter is turned off then back on, the "Auto Power Off" feature will be enabled again.

Backlight


Press the Backlight Button to turn the LCD Backlight on and off.

Beeper Off

To turn the beeper off, press and hold the Backlight button while powering the meter on. The Beeper Off indicator will appear on the LCD. If the meter is turned off then back on, the beeper will be enabled again.

Battery Replacement

1. Loosen the screw at the bottom of the meter and slide the cover away from the meter.
2. Replace the four (4) AA batteries.
3. Reinstall the battery door and tighten the screw to fasten in place.

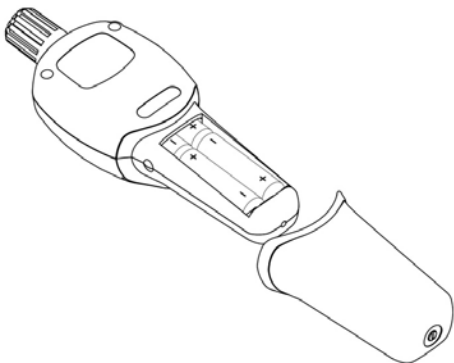

Accessories and Replacement Parts

CA-05A Soft Carrying Case

Don't see your part listed here? For a complete list of all accessories and replacement parts visit your product page on www.REEDInstruments.com.

Applications

- Residential and commercial safety
- Verifying furnaces, cookers, water boilers and gas room heaters

Product Care

To keep your instrument in good working order we recommend the following:

- Store your product in a clean, dry place.
- Change the battery as needed.
- If your instrument isn't being used for a period of one month or longer please remove the battery.
- Clean your product and accessories with biodegradable cleaner. Do not spray the cleaner directly on the instrument. Use on external parts only.

Product Warranty

REED Instruments guarantees this instrument to be free of defects in material or workmanship for a period of one (1) year from date of shipment. During the warranty period, REED Instruments will repair or replace, at no charge, products or parts of a product that proves to be defective because of improper material or workmanship, under normal use and maintenance. REED Instruments total liability is limited to repair or replacement of the product. REED Instruments shall not be liable for damages to goods, property, or persons due to improper use or through attempts to utilize the instrument under conditions which exceed the designed capabilities. In order to begin the warranty service process, please contact us by phone at 1-877-849-2127 or by email at info@REEDInstruments.com to discuss the claim and determine the appropriate steps to process the warranty.

Product Disposal and Recycling



Please follow local laws and regulations when disposing or recycling your instrument. Your product contains electronic components and must be disposed of separately from standard waste products.

Product Support

If you have any questions on your product, please contact your authorized REED distributor or REED Instruments Customer Service by phone at 1-877-849-2127 or by email at info@REEDInstruments.com.

Please visit www.REEDInstruments.com for the most up-to-date manuals, datasheets, product guides and software.

*Product specifications subject to change without notice.
All rights reserved. Any unauthorized copying or reproduction of this manual is strictly prohibited without prior written permission from REED Instruments.*

REED INSTRUMENTS

TEST & MEASURE WITH CONFIDENCE



Access our
Product Catalog

Over 200 portable test and
measurement instruments

