


Insta-Test[®] ANALYTIC


Free & Total Chlorine

25 Test Strips

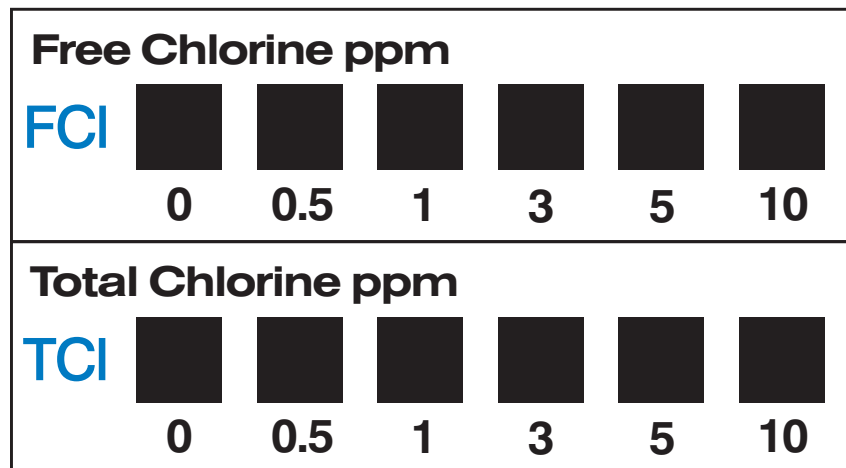

Immerse strip for **2 seconds**.
Remove strip with **pads face up**.
SHAKE ONCE TO REMOVE EXCESS WATER.

Read immediately: FCI > TCI.

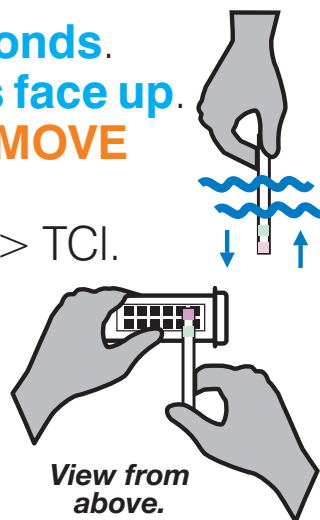

- Keep wet fingers out of the bottle.
- Cap bottle tightly after removing strip.
- Store in a cool, dry place.